

FIG. 1

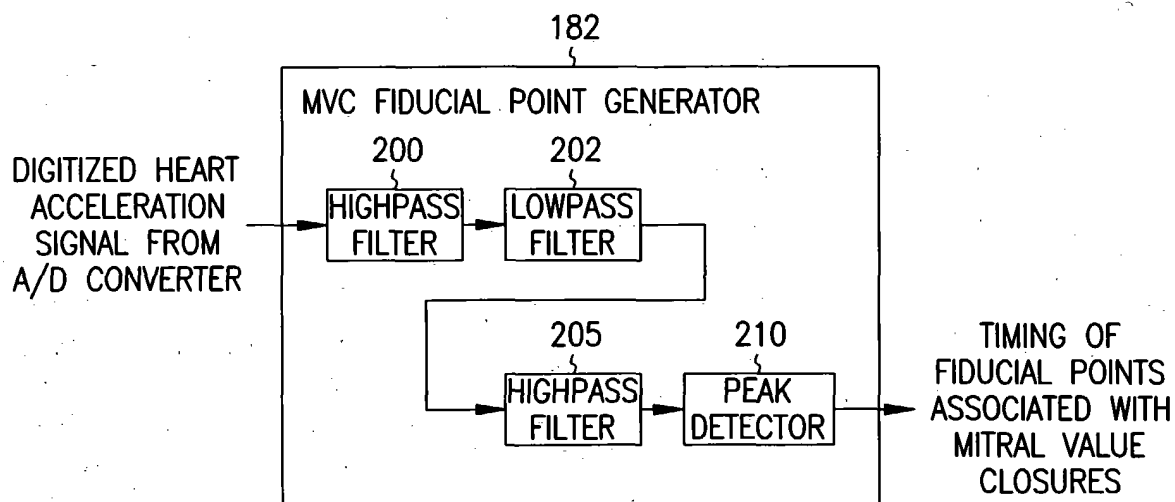


FIG. 2

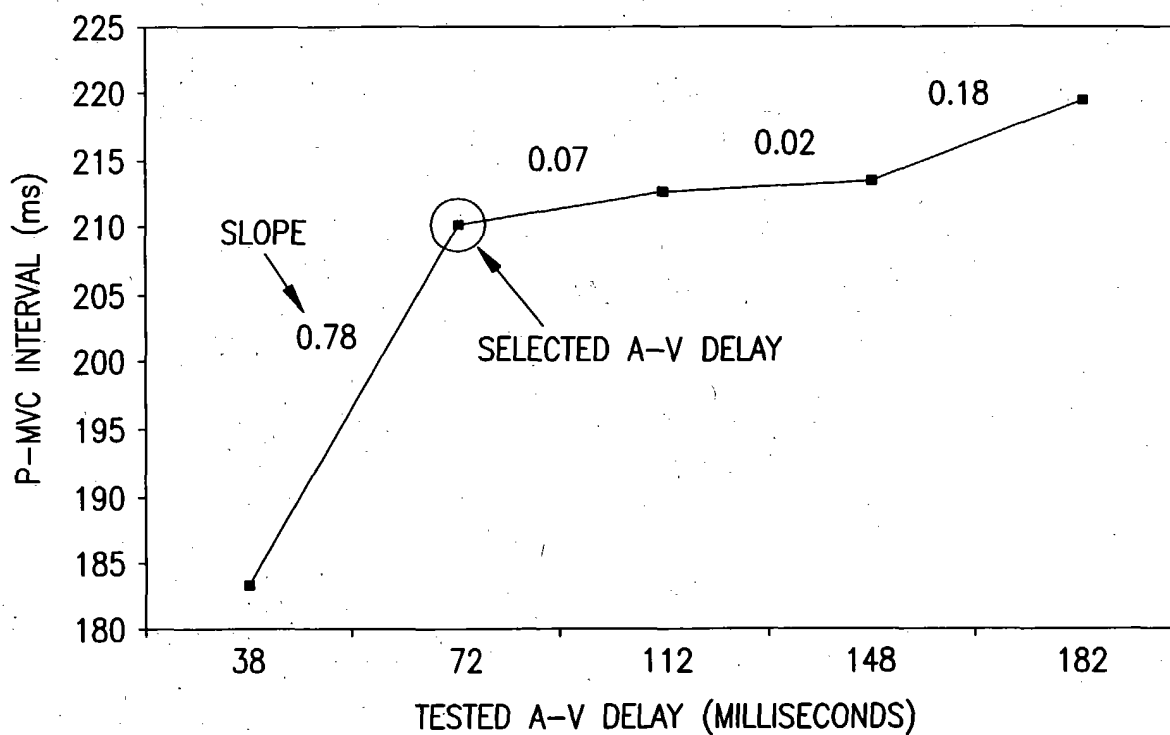


FIG. 3

TITLE: CARDIAC RHYTHM MANAGEMENT SYSTEM SELECTING A-V DELAY BASED ON  
INTERVAL BETWEEN ATRIAL DEPOLARIZATION AND MITRAL VALVE CLOSURE

INVENTORS NAME: William C. Lincoln et al.

Dkt #: 279.360US2

3/5

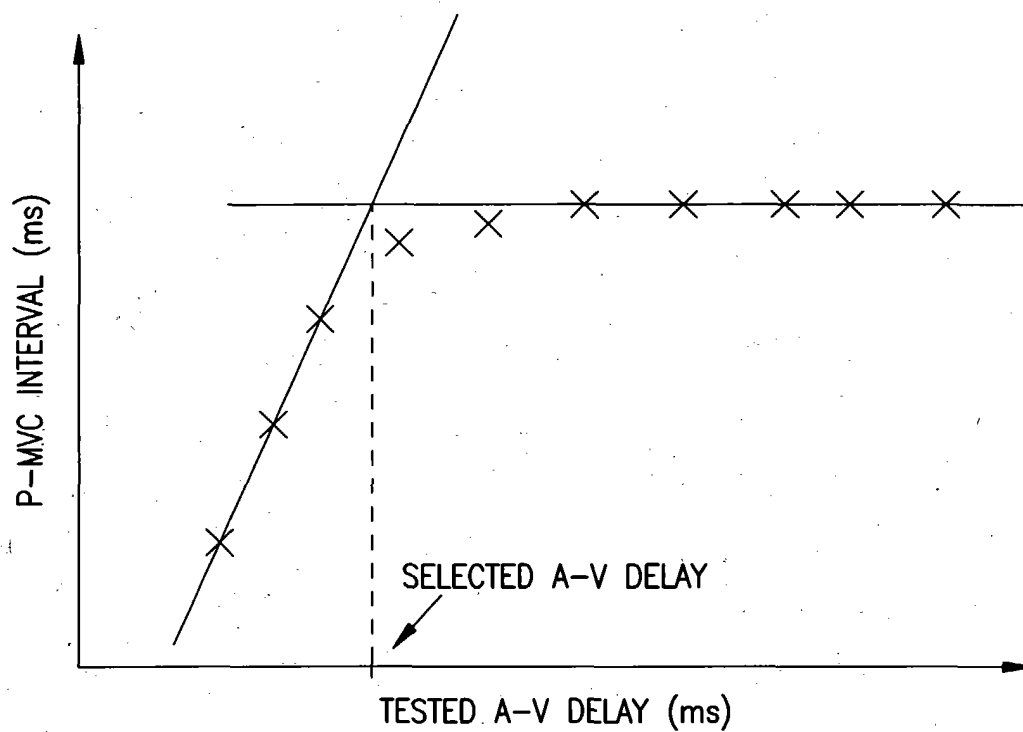


FIG. 4

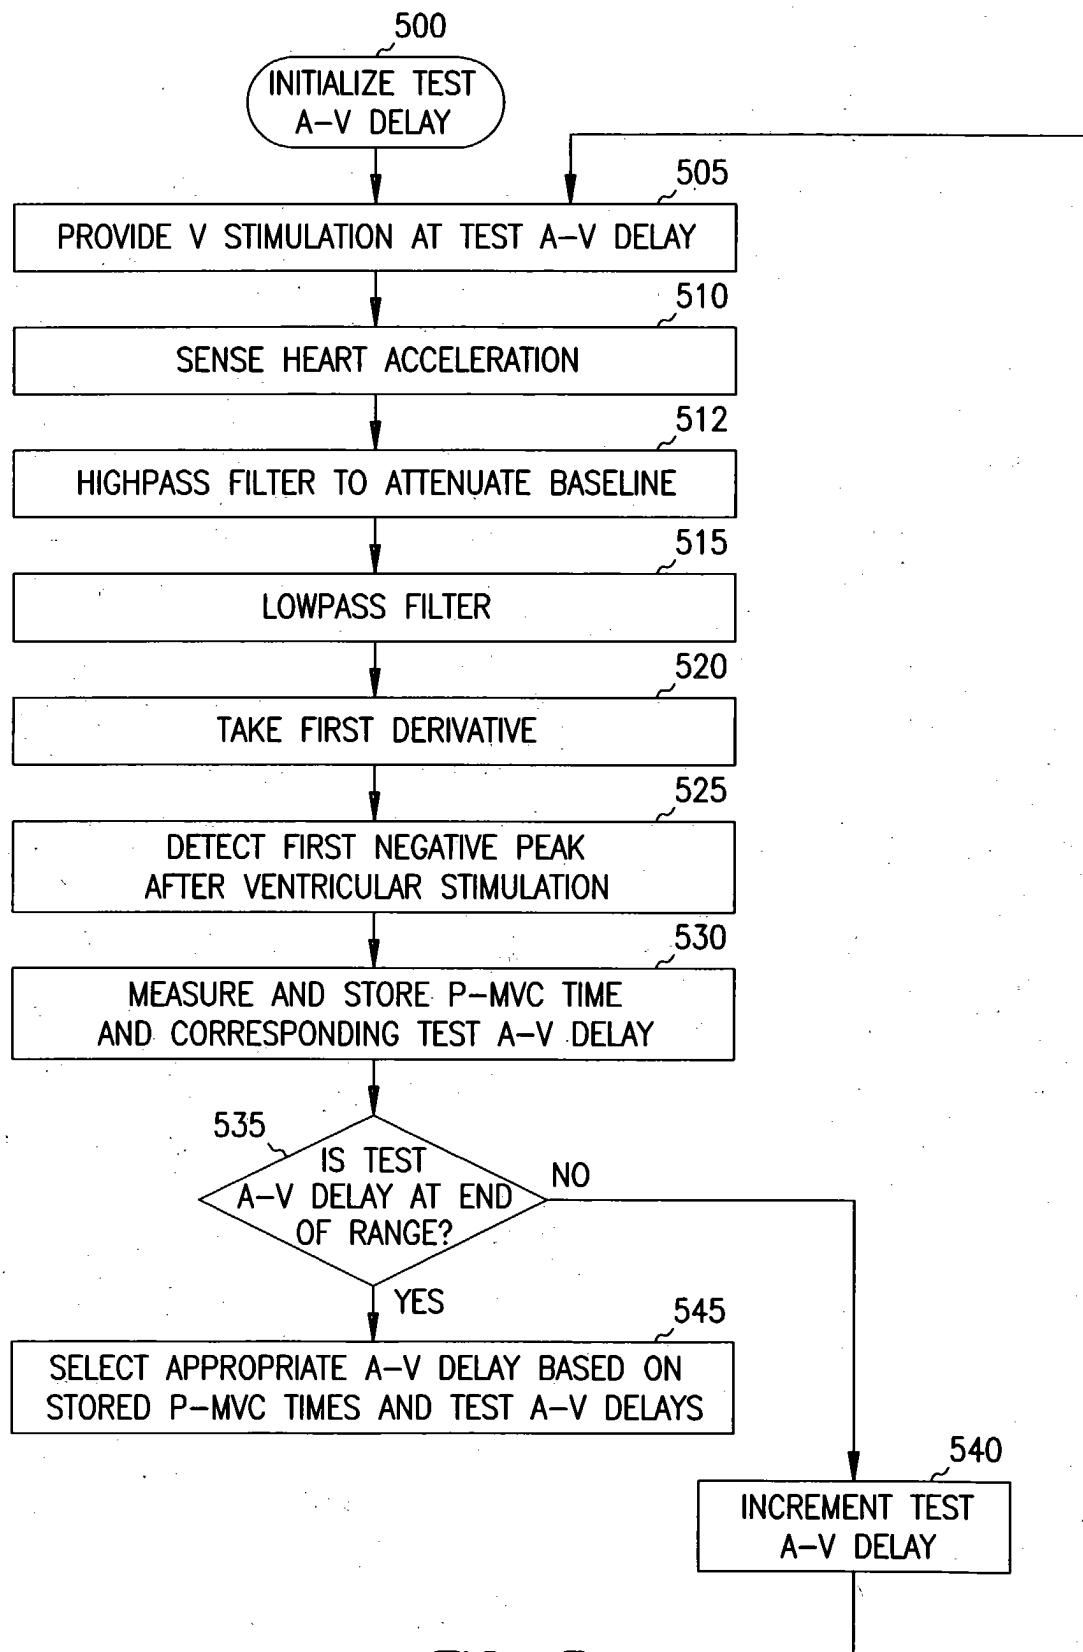


FIG. 5

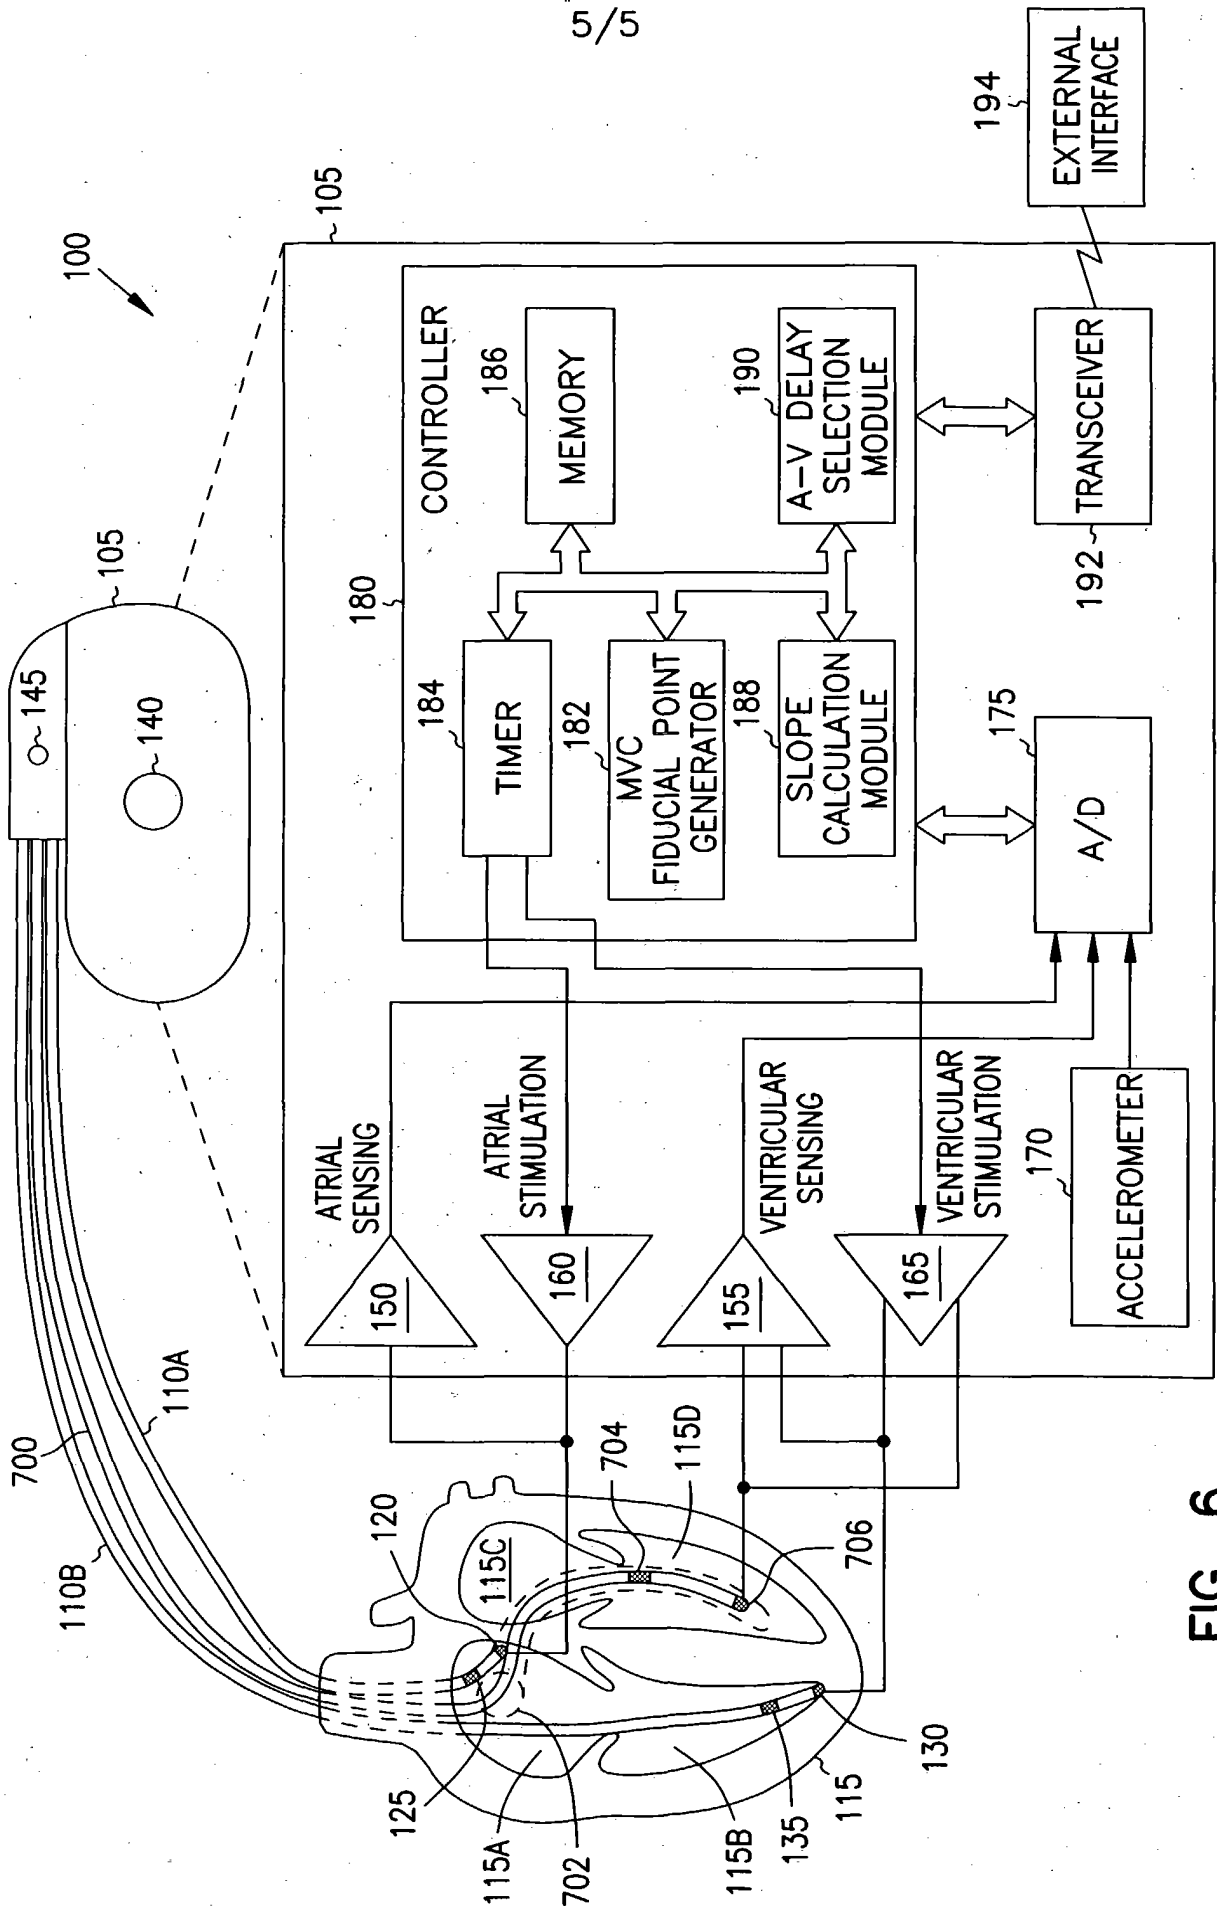


FIG. 6